


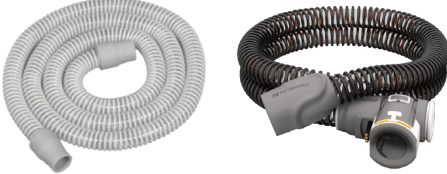





Sleep supplies replacement schedule:

| Timing | Sleep supply | Reason to replace regularly |
|-----------------------|--|---|
| Twice Monthly | Nasal mask cushions & nasal pillows (including oral/nasal combos)  | Cushions/pillows degrade. Replace them for cleanliness, and to keep a good seal and fit. |
| | Disposable filters  | Filters can wear out or clog if not replaced, and can expose you to dust, mold, and germs. |
| Each Month | Full-face mask cushions  | Cushions degrade. Replace them monthly to keep a good seal and comfortable fit. |
| Every 3 Months | Mask frame (excludes headgear)  | Frames break down over time, which affects the fit and therapy. |
| | Tubing (standard or heated)  | Tubes wear down and can start leaking, which decreases therapy effectiveness. |
| Every 6 Months | Headgear and chin straps  | Straps stretch out, losing elasticity — resulting in over-tightening. They can also hold germs. |
| | Humidifier water chamber  | Chambers age, crack, and can grow bacteria or mold. |
| | Non-disposable filters  | Non-disposable filters wear out or clog if not replaced, and can hold dust, mold, and germs. |